


# Axygen® SnapLock Microcentrifuge Tubes

0.6 mL, 1.5 mL, 2.0 mL, 5.0 mL

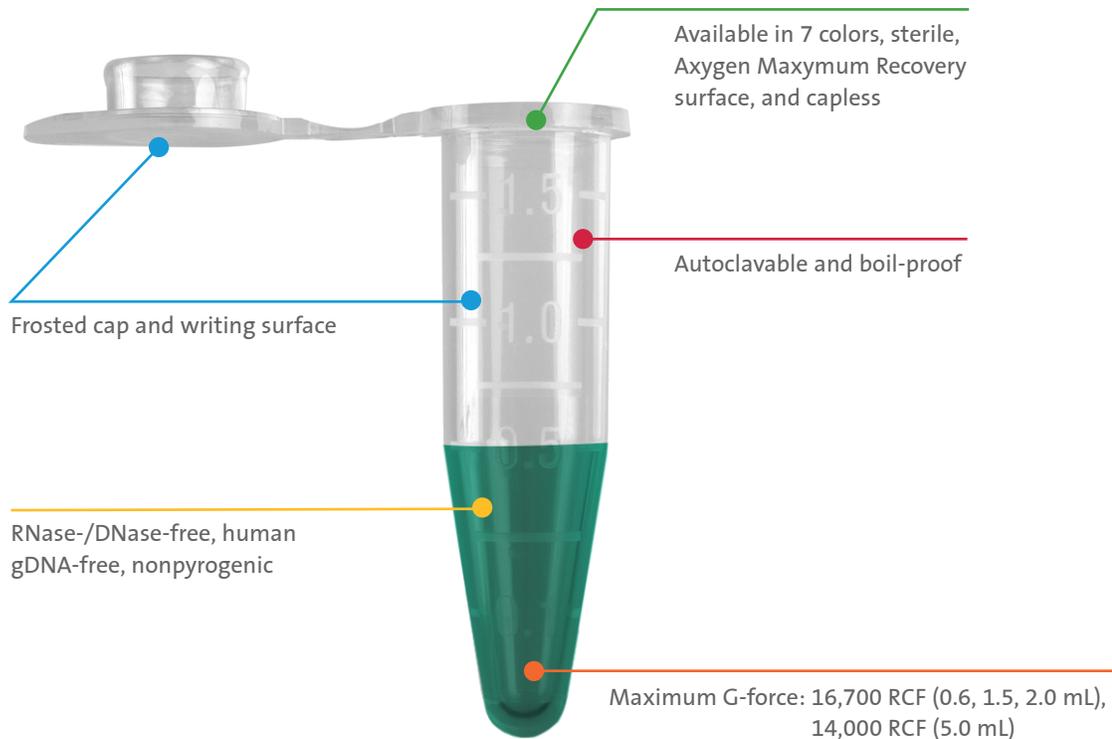

## Ordering Information

*Products may not be available in all markets.*

Cat. No.	Description	Quantity
MCT-060-C	0.6 mL Snaplock microcentrifuge tubes, MaxyClear	1,000/pack, 10 packs/case
MCT-060-C-S	0.6 mL Snaplock microcentrifuge tubes, MaxyClear, sterile	100/bag, 5 bags/pack, 10 packs/case
MCT-150-C	1.5 mL Snaplock microcentrifuge tubes, MaxyClear	5,000/pack, 10 packs/case
MCT-150-C-S	1.5 mL Snaplock microcentrifuge tubes, MaxyClear, sterile	50/bag, 5 bags/pack, 10 packs/case
MCT-200-C	2.0 mL Snaplock microcentrifuge tubes, MaxyClear	5,000/pack, 10 packs/case
MCT-200-C-S	2.0 mL Snaplock microcentrifuge tubes, MaxyClear, sterile	50/bag, 5 bags/pack, 10 packs/case
MCT-500-C	5.0 mL Snaplock microcentrifuge tubes, MaxyClear	250/pack, 5 packs/case
MCT-500-C-S	5.0 mL Snaplock microcentrifuge tubes, MaxyClear, sterile	250/pack, 5 packs/case

**NOTE:** Other options are available, including full cases of different colors, assorted colors in the same case, capless tubes, and tubes with Axygen Maxymum Recovery® surface.

**Warranty/Disclaimer:** Unless otherwise specified, all products are for research use or general laboratory use only.\* Not intended for use in diagnostic or therapeutic procedures. Not for use in humans. These products are not intended to mitigate the presence of microorganisms on surfaces or in the environment, where such organisms can be deleterious to humans or the environment. Corning Life Sciences makes no claims regarding the performance of these products for clinical or diagnostic applications. \*For a listing of US medical devices, regulatory classifications or specific information on claims, visit [www.corning.com/resources](http://www.corning.com/resources).

*Corning's products are not specifically designed and tested for diagnostic testing. Many Corning products, though not specific for diagnostic testing, can be used in the workflow and preparation of the test at the customers discretion. Customers may use these products to support their claims. We cannot make any claims or statements that our products are approved for diagnostic testing either directly or indirectly. The customer is responsible for any testing, validation, and/or regulatory submissions that may be required to support the safety and efficacy of their intended application.*

# CORNING

**Corning Incorporated**  
Life Sciences

[www.corning.com/lifesciences](http://www.corning.com/lifesciences)

## **NORTH AMERICA**

t 800.492.1110  
t 978.442.2200

## **ASIA/PACIFIC**

### **Australia/New Zealand**

t 61 427286832

### **Chinese Mainland**

t 86 21 3338 4338

### **India**

t 91 124 4604000

### **Japan**

t 81 3-3586 1996

### **Korea**

t 82 2-796-9500

### **Singapore**

t 65 6572-9740

### **Taiwan**

t 886 2-2716-0338

## **EUROPE**

[CEurope@corning.com](mailto:CEurope@corning.com)

### **France**

t 0800 916 882

### **Germany**

t 0800 101 1153

### **The Netherlands**

t 020 655 79 28

### **United Kingdom**

t 0800 376 8660

## **All Other European Countries**

t +31 (0) 206 59 60 51

## **LATIN AMERICA**

[grupoLA@corning.com](mailto:grupoLA@corning.com)

### **Brazil**

t 55 (11) 3089-7400

### **Mexico**

t (52-81) 8158-8400